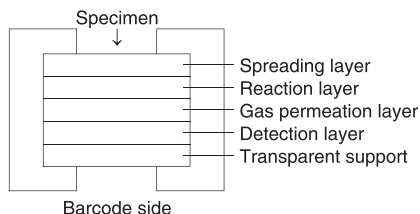


FUJI DRI-CHEM SLIDE NH₃-WII**[Warnings and precautions]**

- Only the required number of slides should be taken out of the refrigerator and warmed up to room temperature before opening the individual packages.
- Do not touch either the center part of the surface or the back of the slide.
- A new slide must be used for each measurement. Do not reuse.
- Handle all patient specimens, control serum and used tips carefully as biohazardous samples. Wear proper gloves, glasses and other protective gear for your safety.
- Used slides are categorized as infectious waste. Make sure to dispose them in accordance with the Waste Disposal Law and other related regulations, which prescribe the proper method of disposal, such as incineration, melting, sterilization or disinfection.

[Composition of the slide]**1. Multi-layered structure****2. Ingredients per slide**

- Bromphenol blue 0.018 mg (0.026 μmol)

[Intended use]

Quantitative measurement of ammonia concentration in whole blood.
For *in vitro* diagnostic use only.

[Principle of the measurement]

10 μL of whole blood is deposited on a FUJI DRI-CHEM SLIDE NH₃-WII. After depositing, the specimen spreads uniformly on the spreading layer and diffuses into the underlying reaction layer, in which solubilized ammonium ion reacts to generate ammonia gas. The color of bromphenol blue in the detection layer is changed from yellow to green or blue by the ammonia gas penetrated from the porous gas permeation layer. The slide is incubated at 37 °C for a fixed time in the FUJI DRI-CHEM ANALYZER and the optical reflection density is measured at 600 nm. The optical reflection density is then converted into the ammonia concentration using a calibration curve preinstalled in the analyzer.

Bromphenol blue + NH₃ → Blue color dye

[Additional special equipment]

Analyzer: FUJI DRI-CHEM ANALYZER
Other implements: FUJI DRI-CHEM QC CARD (attached)
: FUJI DRI-CHEM CLEAN TIPS or FUJI DRI-CHEM AUTO TIPS
: FUJI HEPARIN/PLAIN TUBE or Blood collection tube specified in the "INSTRUCTION MANUAL" for FUJI DRI-CHEM ANALYZER

[Specimen requirements]

- NH₃ concentration is known to increase with time, especially when kept as whole blood. Measure immediately after the blood collection. When the specimen cannot be measured immediately, keep the specimen on ice.
- Heparin-Na/heparin-Li and EDTA salt can be used as the anticoagulant. When using heparin, less than 50 unit of heparin should be used per 1 mL of whole blood. When using EDTA salt, less than 10 mg should be used per 1 mL of whole blood. Do not use heparin ammonium, sodium fluoride, citric acid, oxalic acid and monoiodoacetic acid.
- Do not use kanamycin added blood collection tube.
- When using automatic sampling device of the FUJI DRI-CHEM ANALYZER, mix gently, set the specimen and start immediately.

[Procedure]

- Read in the new QC-card when you switch to a new box of slides.
- Set slides on FUJI DRI-CHEM ANALYZER.
- Set a sample tube in the specified sample rack.
- Input a sequence No. and a sample ID if appropriate.
- Press the "START" key to initiate testing.
For further details of operation procedure, consult "INSTRUCTION MANUAL" for FUJI DRI-CHEM ANALYZER.

[Reference interval]

9–47 μmol/L (12–66 μg/dL as NH₃-N)

As the reference intervals depend on the population of the test, it is required that each laboratory set its own reference intervals. The clinical diagnosis must be made by the doctor in charge based on the measured results in the light of clinical symptoms and other test results.

[Performance characteristics]

1. Dynamic range 7–357 μmol/L (10–500 μg/dL as NH₃-N)

2. Accuracy

Concentration range	Accuracy
7–107 μmol/L	Within ± 16 μmol/L
107–357 μmol/L	Within ± 15 %

3. Precision

Concentration range	Precision
7–107 μmol/L	SD ≤ 6.4 μmol/L
107–357 μmol/L	CV ≤ 6 %

4. Correlation

Correlation was evaluated between NADS* method run on HITACHI automated analyzer and the FUJI DRI-CHEM system. Whole blood measured by FUJI DRI-CHEM system was then centrifuged and the obtained plasma was run on a HITACHI automated analyzer. This examination was carried out at the laboratory of FUJIFILM Corporation.

*NADS: Nicotinamide adenine dinucleotide synthetase

	n	Slope	Intercept	Correlation coefficient
Whole blood and plasma	77	1.044	-2.9	0.999

5. Known interfering substances

- Isopropylamine gives plus bias.
- The effects on the measured value were examined by adding substances as shown below to a serum sample obtained from a healthy volunteer or a control serum. No significant effect was observed to the following concentration for each substance.

Ascorbic acid	0.57 mmol/L
Bilirubin	340 μmol/L
Hemoglobin	5000 mg/L
Hematocrit	20–60 %*

These results are representative;

- Test condition may have some influence on your results.
- Interferences from other substances are not predictable.

*At the normal range of ammonia concentration.

[Internal quality control]

The accuracy and precision of this product can be evaluated with FUJI DRI-CHEM CONTROL QN.

- Measure FUJI DRI-CHEM CONTROL QN in the same way as patient specimens.
- When the results obtained are outside the expected range shown in the sheet attached to FUJI DRI-CHEM CONTROL QN, investigate the cause.
For additional information, consult "Instructions for Use" for FUJI DRI-CHEM CONTROL QN.

[Traceability of calibrators and control materials]

NH₃...CERI (Ammonium ion standard)

Note: This reference material is applied to the reference method of FUJIFILM Corporation and is not directly applicable to FUJI DRI-CHEM SLIDE.

CERI: Chemicals Evaluation and Research Institute, Japan

[Storage and shelf life]

- Storage: This product must be stored between 2–8 °C (35.6–46.4 °F) before use.
- Expiry date is printed on the carton.
- Use immediately after opening the individual package.

[Contents]

: Slide	24
: QC card	1



<http://www.fujifilm.com/products/medical/>



FUJIFILM Europe GmbH
Heesenstrasse 31, 40549 Düsseldorf, GERMANY



FUJIFILM Corporation
26-30, Nishiazabu 2-Chome, Minato-ku, Tokyo 106-8620, JAPAN